



(11) **EP 1 203 592 A1**

(12) **EUROPEAN PATENT APPLICATION**

(43) Date of publication:
08.05.2002 Bulletin 2002/19

(51) Int Cl.7: **A61M 1/36, B01D 19/00**

(21) Application number: **01125951.2**

(22) Date of filing: **31.10.2001**

(84) Designated Contracting States:
AT BE CH CY DE DK ES FI FR GB GR IE IT LI LU
MC NL PT SE TR
 Designated Extension States:
AL LT LV MK RO SI

• **Tiedtke, Hans-Jürgen**
52064 Aachen (DE)
 • **Stevens, Klaus**
52152 Simmerath-Lammersdorf (DE)

(30) Priority: **06.11.2000 US 246200 P**

(74) Representative: **Vetter, Ewald Otto, Dipl.-Ing. et al**
Melssner, Bolte & Partner
Anwaltssozietät
Postfach 10 26 05
86016 Augsburg (DE)

(71) Applicant: **Convergenza AG**
9490 Vaduz (LI)


(72) Inventors:
 • **Plechinger, Hans**
Britisch Columbia, VIC 6J5 (CA)

(54) **Blood conditioning device**

(57) Blood conditioning device (10) for removing bubbles and particles from a stream containing a mixed flow having both particles and bubbles, said device comprising:

a first dynamic separation section (41) for separating bubbles from said mixed flow, generating a flow of particles and blood but free of bubbles;
 a second section (40) coupled to said first section having a filter membrane arranged to intercept the flow of particles and blood generating a flow of blood free of both particles and bubbles.

Fig. 1

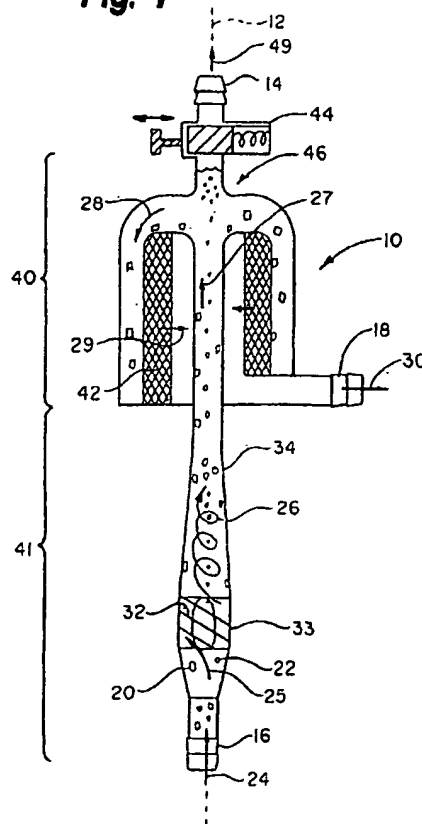

EP 1 203 592 A1

Description**FIELD OF THE INVENTION**

[0001] The present invention relates generally to the extracorporeal circulation of blood during open heart surgery, and more particularly to a device for conditioning blood prior to returning the blood to the patient.

Background of the Invention

[0002] Open heart surgery is performed on a "still" heart. The patient's blood is circulated by an extracorporeal system, which includes a blood pump, a cardiomy reservoir and an oxygenator. In operation, blood is drawn from the patient and pumped through the oxygenator and then returned to the patient. In many instances blood is scavenged from the surgical site and this recovered blood is added to the system through the cardiomy reservoir. As a consequence, surgical debris and air bubbles may be introduced into the system at this point and it is important that the particulate debris and bubbles not be administered to the patient.

[0003] It is the conventional standard of care to place a so-called "arterial filter" in the blood line to intercept and capture particles and gas bubbles before the blood is returned to the patient's body. Filters of this type capture both gas bubbles and particles on a filter mesh. However conventional arterial filters are problematic. Typically the volume of an arterial filter is large to maximize the ability of the device to collect and hold gas bubbles. Captured bubbles are retained on the mesh during the entire surgical procedure. Each bubble that is retained reduces the filter mesh surface area available for particulate collection. It is possible that a large particle load will increase the pressure drop across the filter. This "clogging" effect can increase the pressure on the captured bubbles and force them through the filter. As a consequence of this problem the size of the physical membrane of the arterial filter is very large to provide a margin of safety. However this increases the surface area in contact with blood which is undesirable and increases priming volume which is undesirable. It should also be noted that the mesh size of a typical filter is inadequate to capture small bubbles. Consequently the conventional arterial filter is not efficient at handling bubbles and it is improperly sized for the typical particulate load.

[0004] It must also be noted that blood is a very delicate organ and surface contact, turbulence and pressure drops within the system can injure the blood. These properties of blood must be accommodated as well.

SUMMARY

[0005] In the present invention the blood conditioning device has two main connections. There is a blood input port and a blood output port. A third connection is used to purge or prime the device. In some embodiments of

the device this line is always open and is used for continuous recirculation of blood containing bubble to the cardiomy reservoir.

[0006] The blood conditioning device relies on a first dynamic stage to remove bubbles from the mixed flow of bubbles and particles in blood.

[0007] The dynamic stage passes the bubble free but particle laden blood flow to a second mechanical filter media stage where the particles are trapped. The gas bubbles may be collected and retained in the device or returned with a modest blood flow to the cardiomy reservoir through the third purge or recirculation connection.

[0008] The blood conditioning device is disposable and used once. The particulate debris is retained in the device and discarded at the conclusion of the procedure.

[0009] In the first dynamic stage, the blood is delivered to a blood centrifuge section, which imparts a strong radial acceleration to the blood flow. The pressure gradient is created by forcing the blood along a helical flow path. The radial acceleration causes bubbles both large and small to migrate toward the center streamline of the flow. A bubble pick up may be placed in the zone where the bubbles accumulate. The bubble pick up collects the bubbles and it is connected to the cardiomy reservoir to extract the bubbles from the device. In an alternate embodiment of the device there is no extraction tube or bubble pick off tube and the bubbles are allowed to coalesce and accumulate in the device during operation. This dynamic stage is referred to as the "helix" in the description.

[0010] To purge or prime the device a momentary operation valve is placed on top of the device. The preferred versions of this valve opens side holes in the bubble pick up tube in order to release gross air from the device to the cardiomy reservoir.

BRIEF DESCRIPTION OF THE DRAWINGS

[0011] Throughout the several figures of the drawing identical reference numerals indicate identical structure, wherein:

Fig. 1 is a schematic cross section of a first embodiment of the device;

Fig. 2 is a schematic cross section of a second embodiment of the device;

Fig. 3 is a schematic cross section of a third embodiment of the device;

Fig. 4 is a schematic cross section of a fourth embodiment of the device;

Fig. 5 is a schematic cross section of a fifth embodiment of the device;

Fig. 6A is a schematic cross section of a sixth embodiment of the device;

Fig. 6B is a schematic cross section of a sixth embodiment of the device;

Fig. 7A is a schematic cross section of a seventh embodiment of the device; and,
Fig. 7B is a schematic cross section of a seventh embodiment of the device.

DETAILED DESCRIPTION

[0012] Fig. 1 shows a first embodiment of the blood conditioning device 10. This representative device is shown in a schematic cross section and it is generally symmetric about axis 12. In use this device is mounted vertically with the purge/recirculation port 14 located at the "top". Although the device can be used for conditioning blood in any perfusion circuit it is preferred to couple the input port 16 to the source of blood and to connect the output port 18 directly to the cannula used to deliver blood to the patient. The blood pump supplies the modest pressure difference required to operate the device. The oxygenator and cardiomy reservoir are of conventional design and they are used in the conventional fashion.

[0013] In the various figures the small squares typified by square 20 represent surgical debris with a density slightly greater than blood. The small circles typified by circle 22 represent bubbles or micro bubbles in the blood flow 24. The bubbles have a size of approximately 40mu or more and micro-bubbles have a diameter of 40mu or less. At the inlet port 16, the blood flow 24 has a uniform distribution of particles and bubbles in the input stream, and is called a "mixed blood flow" herein. The mixed blood flow 25 enters an acceleration chamber or "helix" 33 of the dynamic section 41. One or more blades 32 form a helical flow path in the acceleration chamber 33. The blood flow, which leaves the helix 33, has a spiral motion as indicated by blood flow arrow 26. The radial acceleration is strong enough to cause the bubbles to accumulate along the centerline or axis 12 of the device 10. The length of the discharge tube 34 is sufficiently long to permit nearly complete separation of the bubbles from the particles. In this first embodiment of the device these bubbles coalesce and migrate toward zone 46.

[0014] Eventually the spiral motion of the blood flow is reduced as indicated by blood flow 27 and the bubble free blood flow 28, leaves the dynamic section 41 and turns to enter the mechanical separation section 40.

[0015] The blood now free of bubbles enters a flow path that intercepts a membrane 42. The annular membrane 42 filters the blood flow and the particles adhere to the surface of the membrane while the blood passes through the membrane as depicted by blood flow 29. The blood accumulated behind the membrane 42 is delivered to the output port 18 and the now conditioned blood flow 30 is introduced into the patient.

[0016] In operation the particles and blood turn into the mechanical separation section 40 while the buoyancy of the bubbles causes them to coalesce into larger bubble and form a bubble rich volume or zone 46 trapped near the stopcock 44. The purge stopcock 44

may be used to prime the device during setup and may be used to periodically return the bubble rich accumulated volume 46 to the blood cardiomy reservoir during operation.

[0017] Fig. 2 is a schematic cross section of a second embodiment of the blood conditioning device 10. In this second embodiment a bubble pick off tube 48 is positioned to intercept the stream of micro-bubbles from the dynamic section 41. The opening 47 of the bubble pick off tube 48 is sized to capture the blood flow near the centerline 12 of the dynamic section. The opening 47 establishes a small regulated blood flow 49 from the device to the cardiomy reservoir (not shown) which carries the bubbles back to the cardiomy reservoir. This recirculation line 13 is always open.

[0018] Fig. 3 is an alternate embodiment incorporating a bubble pick off 48 which pulls bubbles from the device through opening 47. In this device operates similar to figure 2 but in contrast the particles can directly engage the filter mesh 42 as the blood flow flows in an outward direction from the center of the device.

[0019] Fig. 3 also shows the preferred form of momentary operation valve 50. The momentary operation valve 50 is provided at the top of the housing to allow the user to purge or prime the device. When "open" the valve 50 allows the gross air from the interior volume of the device to be purged into the cardiomy reservoir. When closed the interior volume of the device is closed off but the bubble pick off tube remains open to the cardiomy reservoir.

[0020] The preferred form of the valve includes a ring 51 which can slide between two positions. In the first position the ring covers side holes 47 in the bubble pick up tube 48 and is in the "dosed" position. The valve 50 in Fig. 7A is shown in this state. In the second "open" position the ring 51 uncovers the side holes 47 in the bubble pick off tube 48 as seen in the Fig. 3 among others. In the "open" position the interior volume of the housing 13 is open to the reservoir.

[0021] This valve may be operated to bleed the system both prior to use and during a surgery. In general the valve 50 is closed and remains open only while operated by the perfusionist.

[0022] Fig. 4 is an alternate embodiment of the invention which includes a diverging channel 53 to decrease the velocity of the blood flow after the bubbles have been picked off at opening 47. It is expected to be advantageous to decrease the velocity in the mechanical filtration section 40.

[0023] Fig. 5 is an alternate embodiment of the device having a "side by side" configuration the dynamic section 41 located substantially next to the mechanical filtration section 40. The principle advantage of this configuration is the ability to see the bubble pick off 48 and related area of the dynamic section during operation and provides more options for flow dynamic optimization in the two sections.

[0024] Fig. 6A is side elevation of an alternate embod-

iment of the device. In this configuration the device is very compact. In this version of the device the particles 20 are captured on the outer surface of the annular filter mesh 42, while the bubbles pass the helix 33 in advance and are picked up in line 48. On top of the device the preferred momentary operation valve 50 is schematically shown, opening side hole to the recirculation line to release gross air upon operation.

[0025] Fig. 6B is top view of an alternate embodiment of the device. In this view one can see that the helix 33 is located in a circular flow path. In general the input mixed blood flow 24 turns through about 90 degrees before it enters the helix 33.

[0026] The dynamic section 41 extends around the circle and the bubble pick off 48 is downstream through another 90 degrees of turning.

[0027] Fig. 7A is side elevation of an alternate embodiment of the device. In this embodiment in contrast to figure 6 the blood flow carrying particulates is from the interior of the device to the exterior as typified by the location of particle 20. In this embodiment conical surface or funnel is used to accelerate blood flow as it enters the filter zone.

[0028] Fig. 7B is top view of an alternate embodiment of the device. In this version of the device the helix 33 is located part way round the circumference of the device with a bubble pick off 48 located downstream of the helix 33.

a mechanical filtration section coupled to said helical blood acceleration section, receiving said acceleration section output flow and for trapping particles carried by said flow producing a device output flow for a patient.

4. The device of claim 3 wherein the dynamic section includes a helical flow path and a bubble pick off tube place to remove bubbles; said bubble pick off tube coupled to the third port and having a continuous recirculation flow during operation of the device.

Claims

1. A blood conditioning device for removing bubbles and particles from a stream containing a mixed flow having both particles and bubbles, said device comprising:

a first dynamic separation section for separating bubbles from said mixed flow, generating a flow of particles and blood but free of bubbles; a second section coupled to said first section having a filter membrane arranged to intercept the flow of particles and blood generating a flow of blood free of both particles and bubbles.

2. The device of claim 1 wherein said dynamic separation section includes a helical flow path for imparting rotary motion to blood flow through the section.

3. A blood conditioning device comprising:

a housing having a first blood inlet port, a second blood outlet port and a third purge/recirculation port; a helical blood acceleration section coupled to said first blood inlet port for removing bubbles from the blood entering the inlet, and producing an acceleration section output flow;

Fig. 1

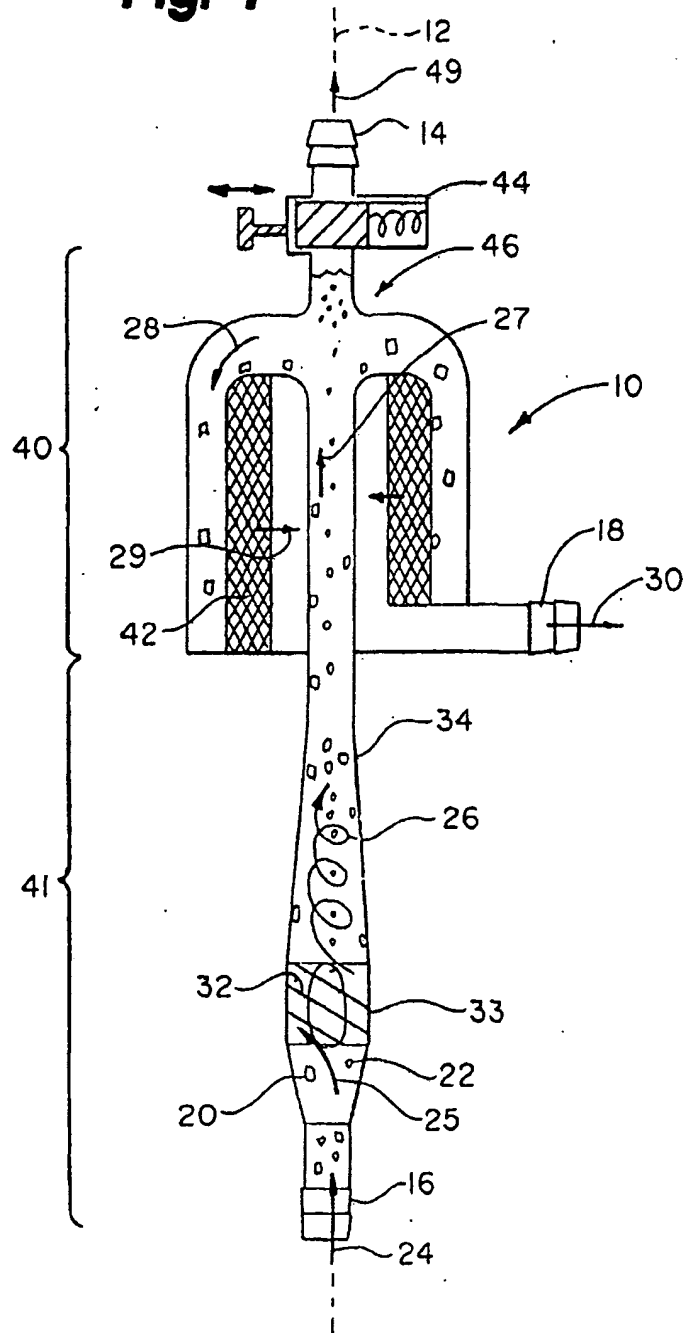


Fig. 2

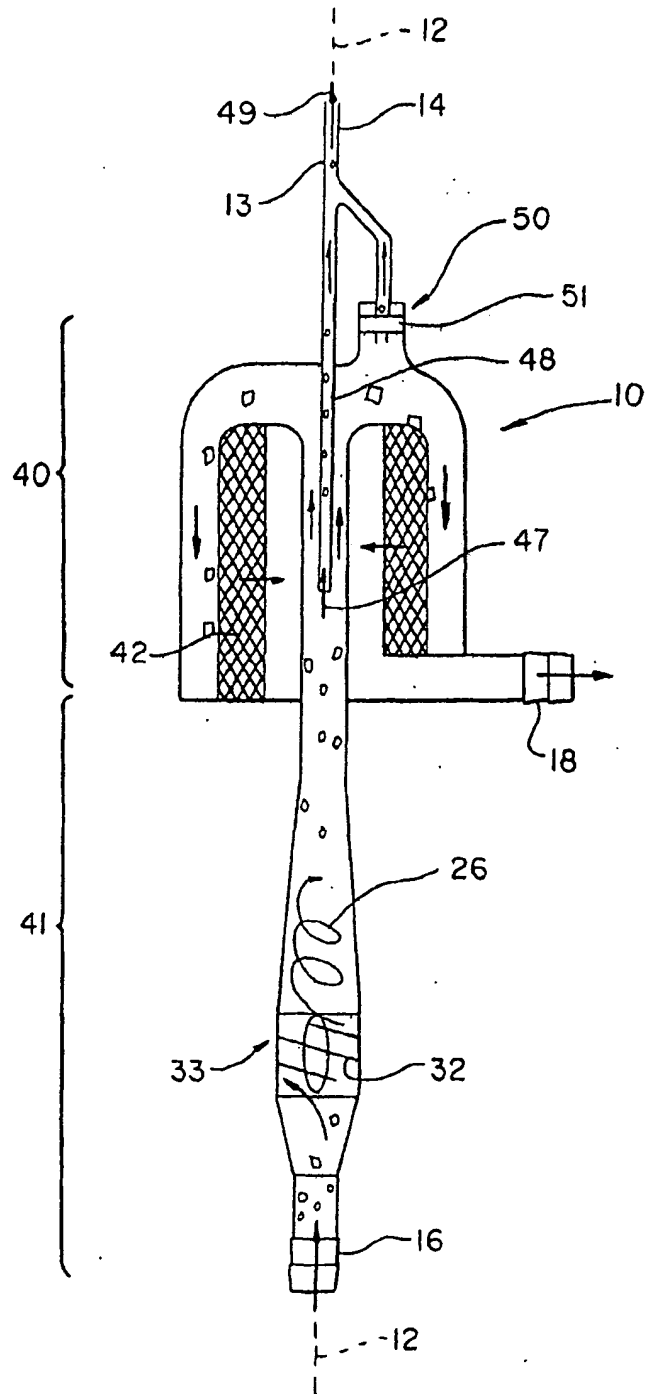


Fig. 3

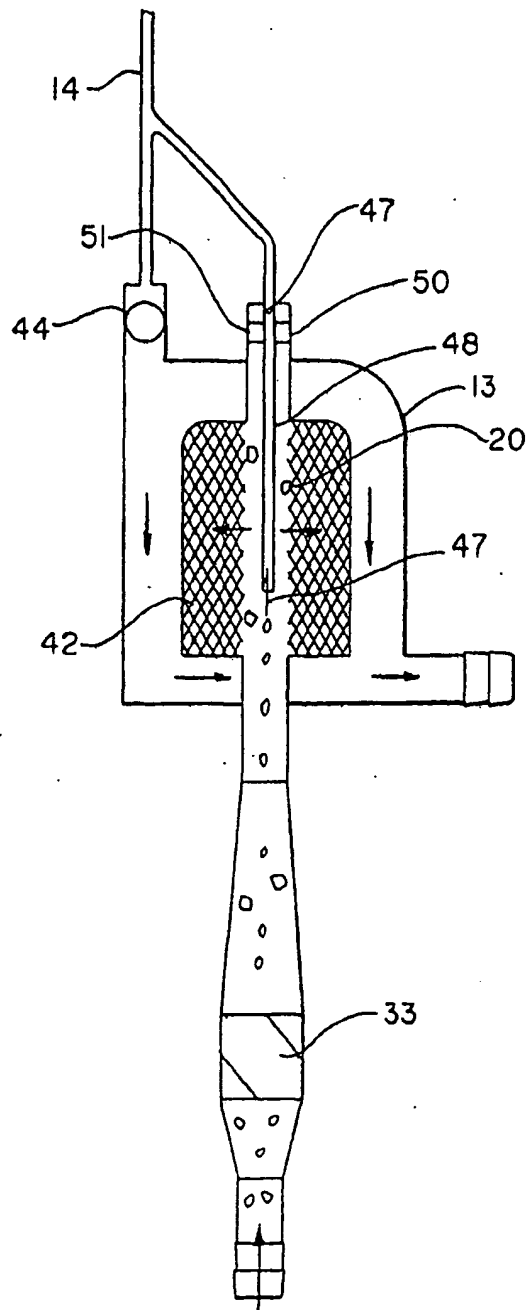


Fig. 4

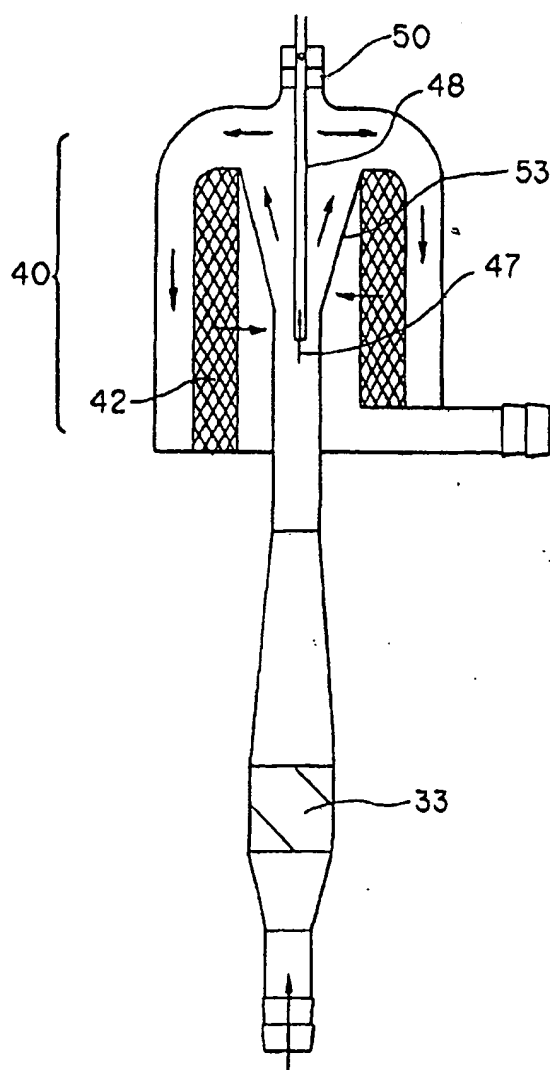


Fig. 5

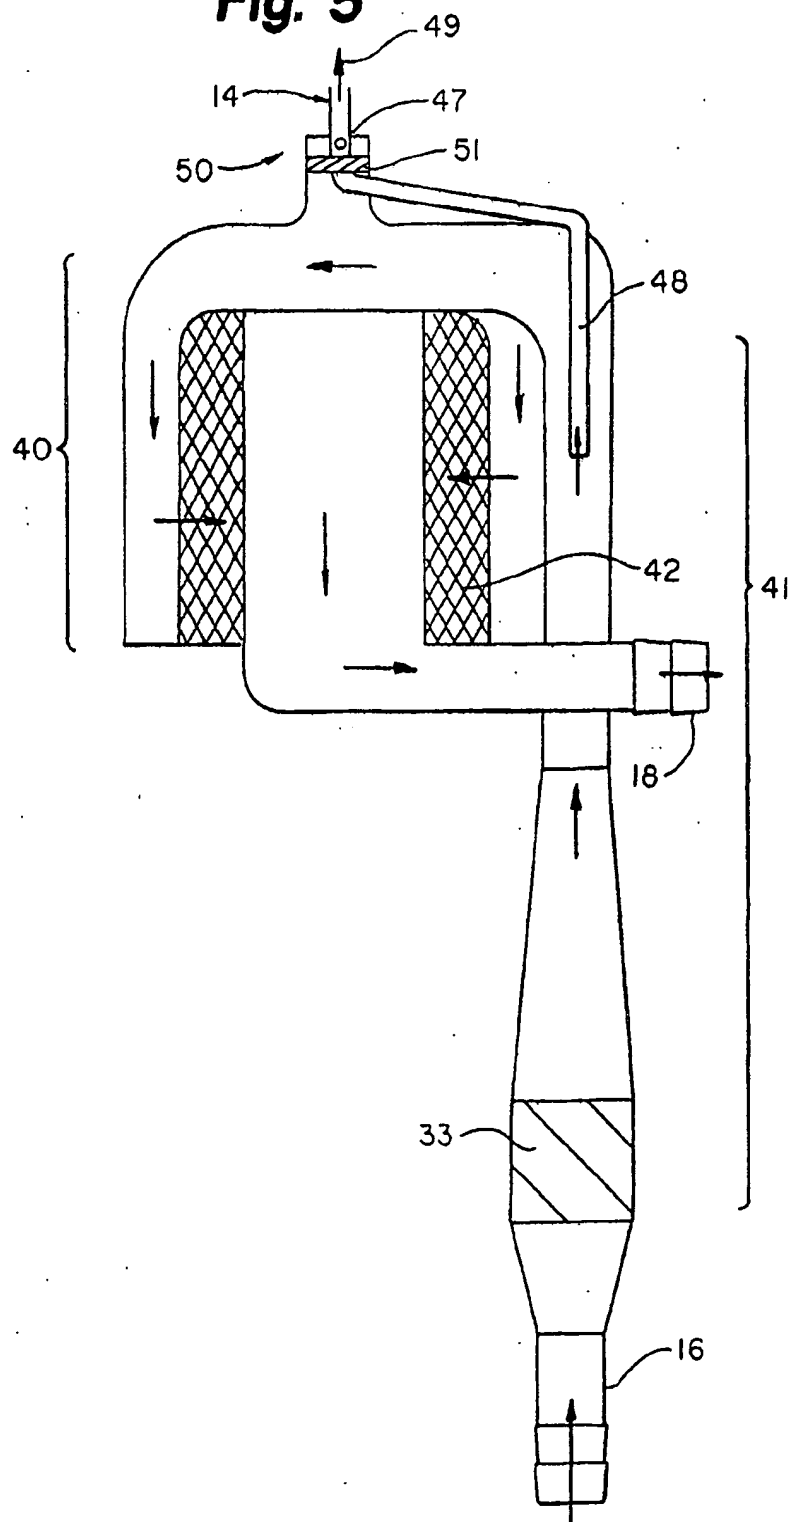


Fig. 6A

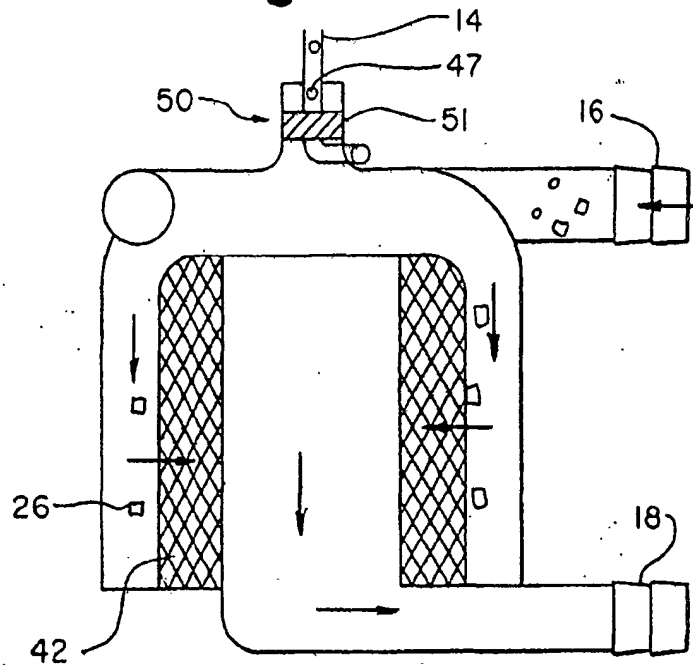


Fig. 6B

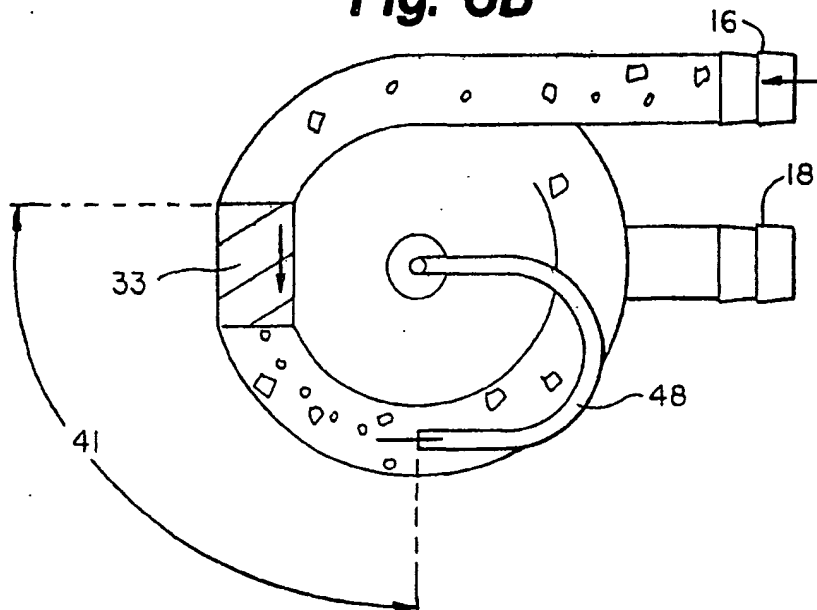


Fig. 7A


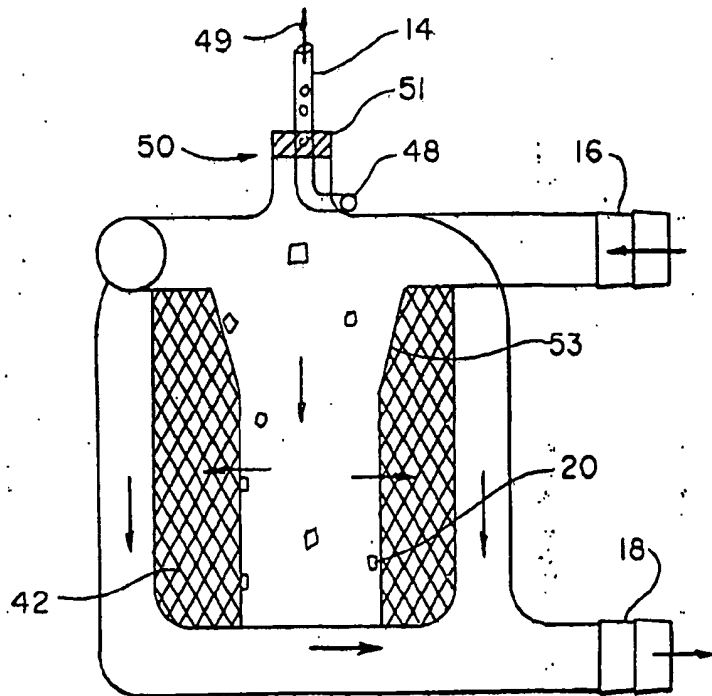


Fig. 7B



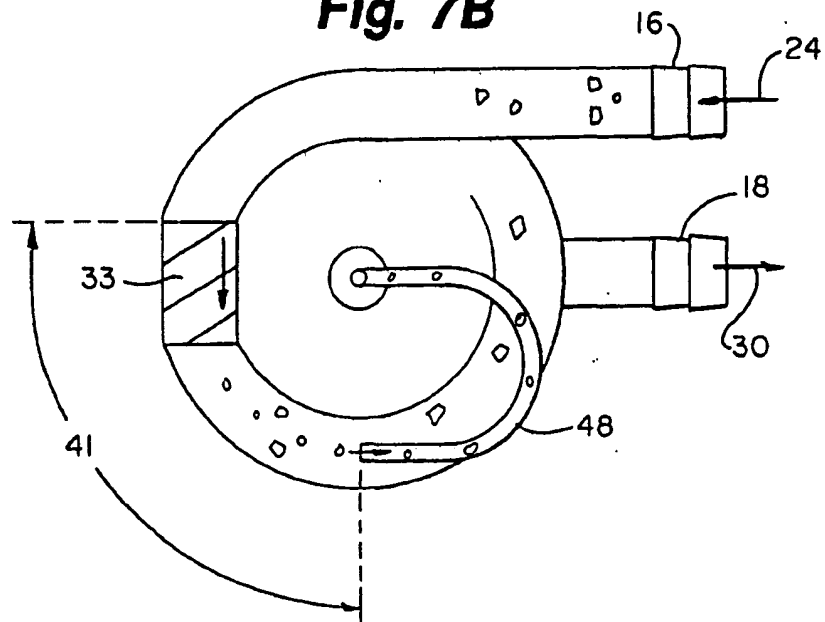

European Patent
Office

EUROPEAN SEARCH REPORT

Application Number
EP 01 12 5951

DOCUMENTS CONSIDERED TO BE RELEVANT			
Category	Citation of document with indication, where appropriate, of relevant passages	Relevant to claim	CLASSIFICATION OF THE APPLICATION (Int.Cl.7)
X	US 6 053 967 A (HEILMANN KLAUS ET AL) 25 April 2000 (2000-04-25) * column 2, line 49 - column 3, line 14 * * column 4, line 5 - column 5, line 12 * * column 6, line 19-22 * * column 5, line 20-23 * * figure 1 *	1,2	A61M1/36 B01D19/00
Y	---	1-4	
Y	WO 00 61208 A (CONVERGENZA AG) 19 October 2000 (2000-10-19) * abstract * * page 2, paragraph 1 * * page 3, paragraph 3 * * page 5, paragraph 2 * * figure 1 *	3,4	
Y	US 5 824 212 A (BROCKHOFF ALEXANDER) 20 October 1998 (1998-10-20) * column 1, line 65 - column 2, line 5; figures 6,7 * * column 5, line 4-20 *	1,2	
			TECHNICAL FIELDS SEARCHED (Int.Cl.7)
			A61M B01D B04C
The present search report has been drawn up for all claims			
Place of search: MUNICH		Date of completion of the search: 11 February 2002	Examiner: Bichlmayer, K-P
<p>CATEGORY OF CITED DOCUMENTS</p> <p>X : particularly relevant if taken alone Y : particularly relevant if combined with another document of the same category A : technological background O : non-written disclosure P : intermediate document</p> <p>T : theory or principle underlying the invention E : earlier patent document, but published on, or after the filing date D : document cited in the application I : document cited for other reasons & : member of the same patent family, corresponding document</p>			

EPO FORM 1503 (03.02) (P04C01)

**ANNEX TO THE EUROPEAN SEARCH REPORT
ON EUROPEAN PATENT APPLICATION NO.**

EP 01 12 5951

This annex lists the patent family members relating to the patent documents cited in the above-mentioned European search report.
The members are as contained in the European Patent Office EDP file on
The European Patent Office is in no way liable for these particulars which are merely given for the purpose of information.

11-02-2002

Patent document cited in search report		Publication date	Patent family member(s)		Publication date
US 6053967	A	25-04-2000	DE	4329385 A1	02-03-1995
			DE	19506506 A1	29-08-1996
			DE	59403215 D1	31-07-1997
			EP	0646380 A1	05-04-1995
			ES	2106420 T3	01-11-1997
			JP	7204408 A	08-08-1995
WO 0061208	A	19-10-2000	WO	0061208 A1	19-10-2000
			EP	1165158 A1	02-01-2002
US 5824212	A	20-10-1998	DE	19545404 A1	12-06-1997
			AT	185276 T	15-10-1999
			DE	59603277 D1	11-11-1999
			EP	0778031 A1	11-06-1997
			ES	2136931 T3	01-12-1999

EPO FORM P0459

For more details about this annex : see Official Journal of the European Patent Office, No. 12/82

**This Page is Inserted by IFW Indexing and Scanning
Operations and is not part of the Official Record**

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images include but are not limited to the items checked:

- ☐ BLACK BORDERS
- ☐ IMAGE CUT OFF AT TOP, BOTTOM OR SIDES
- ☐ FADED TEXT OR DRAWING
- ☐ BLURRED OR ILLEGIBLE TEXT OR DRAWING
- ☐ SKEWED/SLANTED IMAGES
- ☒ COLOR OR BLACK AND WHITE PHOTOGRAPHS
- ☐ GRAY SCALE DOCUMENTS
- ☒ LINES OR MARKS ON ORIGINAL DOCUMENT
- ☐ REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY
- ☐ OTHER: _____

IMAGES ARE BEST AVAILABLE COPY.

As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.